


← Kindergarten

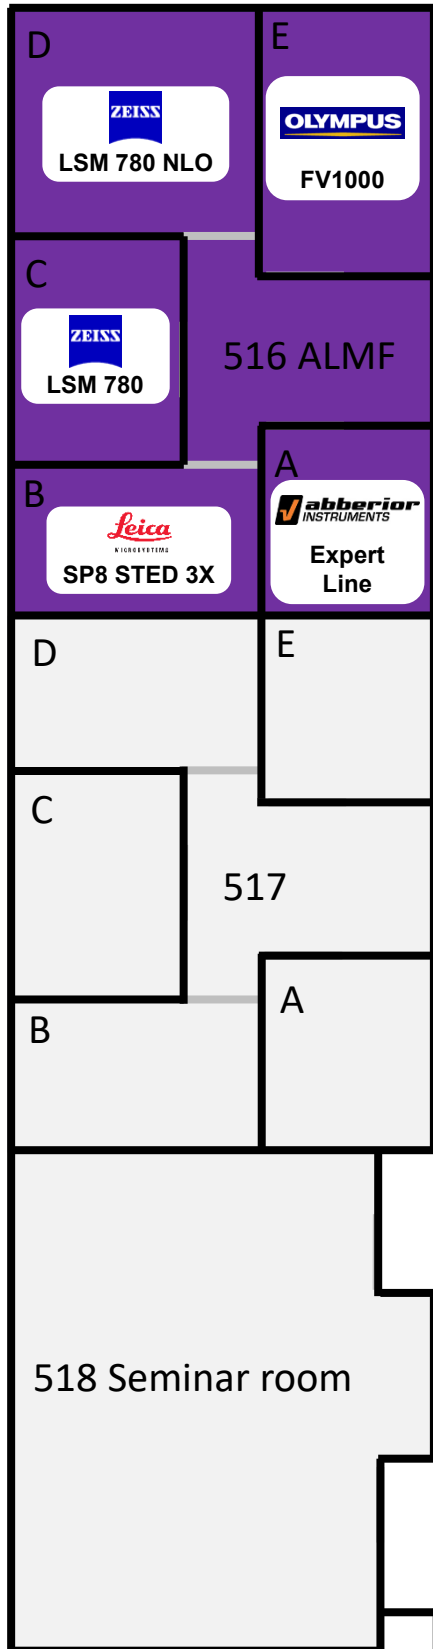

Fluorescent protein room color coding

508 ALMF High-throughput microscopes

B/C

Molecular Devices IXM XLS

Nikon Ti-E platel.

OLYMPUS ScanR C4+5

A

BIO-RAD Spotter

D

ZEISS MicroBeam

E

Nikon Ti-2 PFS

F

Leica SP5 A

B

Nikon A1R

C

OLYMPUS Spin SR

D

ZEISS Cellobservr

B

ZEISS LSM 880 AIRY

C

ZEISS Elyra 7

D

PerkinElmer VoX

A

ZEISS LSM 900

515 ALMF

E

OLYMPUS TIRF

A

Nikon Ti-E PFS

514 ALMF

E

OLYMPUS FV3000

572 WC for disabled

570 WC ladies

571 WC gents

510 Tea Kitchen

512 Beta Test

513 ALMF Storage

B

LUXENDO MuVi SPIM

C

Leica SP8 DLS

D

Leica SR GSD

A

OLYMPUS Safe360

509 ALMF

E

LUXENDO InVi SPIM

501 ALMF Workstations Visitors

502 ALMF Office

503 ALMF Office

504 ALMF Office

505 ALMF Cell Culture

506 ALMF Office

507 ALMF Preparation